Print on Plain White Paper (Part No. 122919)

MIDMARK®

Installation/Operation Instructions

9A82001 SPECIAL PROCEDURES ARMBOARD

KIT COMPONENTS

Part Number	Description	Qty.
9A82001	Procedures Armboard	1
003-0374-00	Installation / Operation Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To provide positioning and restraint for arm during minor procedures on a hand.

WARNING

Mount 9A82001 on siderail bar of exam table. Do not operate table with this accessory installed. Do not use with any other accessories on same side of table. Always support Armboard assembly when changing its position. Assure all positions are solidly locked to prevent sudden movement during procedure.

INSTALLATION

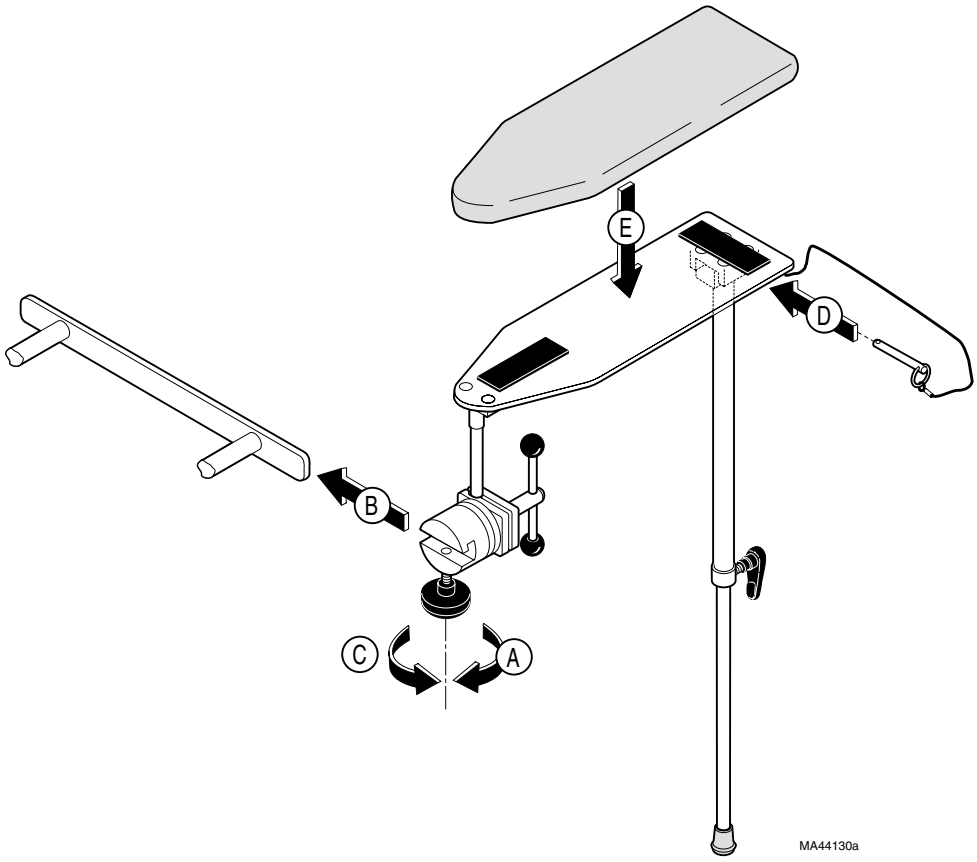

EQUIPMENT ALERT

Place table in desired position before mounting 9A82001 Special Procedures Armboard. To prevent damage to the table or armboard do not operate the table after the Armboard has been installed

A. Loosen knob.
B. Slide swivel block onto side rail to desired position.
C. Tighten knob.
D. Position leg assembly in location on leg brace and insert pin assembly.
E. Install cushion.

OPERATION
(ROTATIONAL POSITIONING)

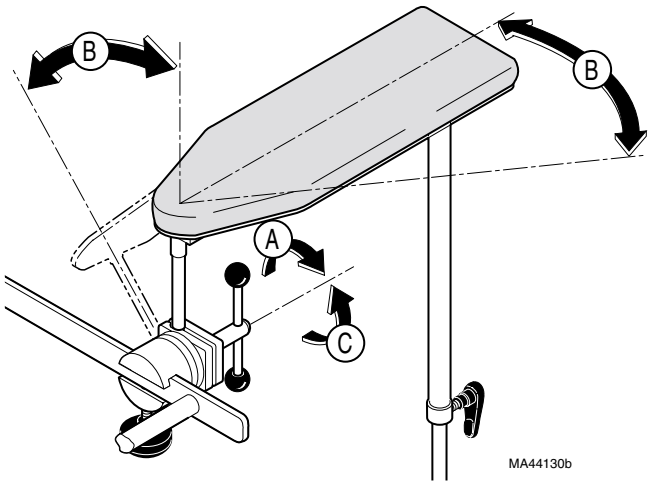

A. Supporting Armboard, loosen T-handle
B. Rotate Armboard to desired position.
C. Tighten T-handle.

OPERATION
(HEIGHT ADJUSTMENT)

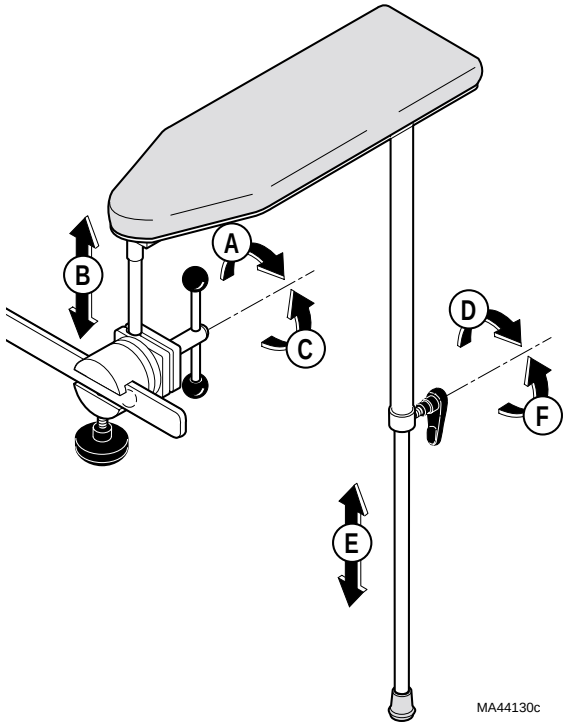

A. Supporting Armboard, loosen T-handle.
B. Raise or lower Armboard to desired position.
C. Tighten T-handle.
D. Loosen knob.
E. Position lower leg in desired position.
F. Tighten knob.

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.

003-0374-00 Rev. D (4/98)